

DuraFlow™ 2 CHRONIC HEMODIALYSIS CATHETER INSTRUCTIONS FOR USE

INDICATIONS FOR USE:

- The DuraFlow™ 2 Hemodialysis Catheter is indicated for use in attaining Long-Term vascular access for Hemodialysis and Apheresis.
- It may be inserted percutaneously and is primarily placed in the internal jugular vein of an adult patient.
- Alternate insertion sites include subclavian vein as required.
- Catheters greater than 40 cm are intended for femoral vein insertion.
- This catheter is indicated for > 30 days long term placement.
- The Valved Peelable Introducer is intended for use in the percutaneous insertion of catheters in the venous system.

CONTRAINDICATIONS:

- The catheter is intended for Long-Term vascular access only and should not be used for any purpose other than indicated in these instructions.

The valved peelable introducer sheath is not designed for use in the arterial system

DESCRIPTION:

- The DuraFlow™ 2 Hemodialysis Catheter is manufactured from soft radiopaque Durathane® material that provides increased patient comfort while providing excellent biocompatibility.



POTENTIAL COMPLICATIONS:

Air Embolus	Lumen Thrombosis
Bacteremia	Mediastinal Injury
Brachial Plexus Injury	Perforation of the Vessel
Cardiac Arrhythmia	Pleural Injury
Cardiac Tamponade	Pneumothorax
Central Venous Thrombosis	Retroperitoneal Bleed
Endocarditis	Right Atrial Puncture
Exit Site Infection	Septicemia
Exsanguination	Subclavian Artery Puncture
Femoral Artery Bleed	Subcutaneous Hematoma
Femoral Nerve Damage	Superior Vena Cava Puncture
Hematoma	Thoracic Duct Laceration
Hemorrhage	Tunnel Infection
Hemothorax	Vascular Thrombosis
Inferior Vena Cava Puncture	Venous Stenosis
Laceration of the Vessel	

- Before attempting the insertion, ensure that you are familiar with the above complications and their emergency treatment should any of them occur.

WARNINGS:

- In the rare event that a hub or connector separates from any component during insertion or use, take all necessary steps and precautions to prevent blood loss or air embolism and remove catheter.

- Do not advance the guidewire or catheter if unusual resistance is encountered.

- Do not insert or withdraw the guidewire forcibly from any component. The wire may break or unravel. If the guidewire becomes damaged, the introducer needle or sheath introducer and guidewire must be removed together.

- Use of excessive pull force on the catheter may cause the suture wing to detach from the bifurcate.

- Federal Law (USA) restricts the device to sale by or on the order of a physician.

- This catheter is for Single Use Only.



- Do not re-sterilize the catheter or accessories by any method.

- The manufacturer shall not be liable for any damages caused by reuse or re-sterilization of this catheter or accessories.

- Contents sterile in unopened, undamaged package.

STERILIZED BY ETHYLENE OXIDE

STERILE EO

- Do not use catheter or accessories if package is opened or damaged.

- Do not use catheter or accessories if any sign of product damage is visible.

- Reuse of single use devices creates a potential risk of patient or user infections. Contamination of the device may lead to injury, illness, or death of the patient.

- Reprocessing may compromise the integrity of the device and/or lead to device failure.

CATHETER PRECAUTIONS:

- Do not use sharp instruments near the extension tubing or catheter lumen.

- Do not use scissors to remove dressing.

- Catheter will be damaged if clamps other than what is provided with this kit are used.

- In the event a clamp breaks, replace the catheter at the earliest opportunity.

- Clamping of the tubing repeatedly in the same location may weaken tubing. Avoid clamping near the luer and hub of the catheter.

- Examine catheter lumen and extensions before and after each treatment for damage.


- To prevent accidents, assure the security of all caps and bloodline connections prior to and between treatments.

- Use only Luer Lock (threaded) Connectors with this catheter.


- Repeated over tightening of bloodlines, syringes, and caps will reduce connector life and could lead to potential connector failure.

INSERTION SITES:

- The patient should be in a modified Trendelenburg position, with the upper chest exposed and the head turned slightly to the side opposite the insertion area. A small rolled towel may be inserted between the shoulder blades to facilitate the extension of the chest area.

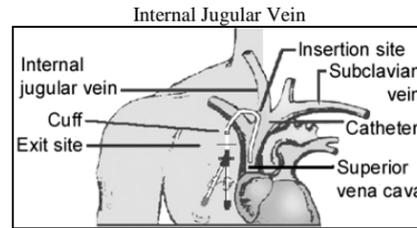

- Have patient lift his/her head from the bed to define the sternomastoid muscle. Catheterization will be performed at the apex of a triangle formed between the two heads of the sternomastoid muscle. The apex should be approximately three fingerbreadths above the clavicle. The carotid artery should be palpated medial to the point of catheter insertion.

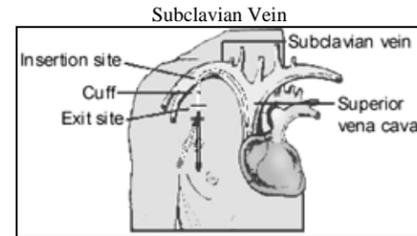


- Note the position of the subclavian vein, which is posterior to the clavicle, superior to the first rib, and anterior to the subclavian artery. (At a point just lateral to the angle made by the clavicle and the first rib.)

WARNING:


- Patients requiring ventilator support are at increased risk of pneumothorax during subclavian vein cannulation, which may cause complications.

- Extended use of the subclavian vein may be associated with subclavian vein stenosis.

Tip Placement



Femoral Vein



- The patient should lie completely on his/her back. Both femoral arteries should be palpated for site selection and consequence assessment. The knee on the same side of the insertion site should be flexed and the thigh abducted. Place the foot across the opposite leg. The femoral vein is then posterior/medial to the artery.

Caution: The incidence of infection may be increased with femoral vein insertion.

- Confirm final position of catheter with chest x-ray. Routine x-ray should always follow the initial insertion of this catheter to confirm proper tip placement prior to use.

- Femoral Catheter tip placement is recommended at the junction of the iliac vein and the inferior vena cava.

DIRECTIONS FOR SELDINGER INSERTION

- Read instructions carefully before using this device. The catheter should be inserted, manipulated, and removed by a qualified, licensed physician or other qualified health care professional under the direction of a physician.

- The medical techniques and procedures described in these instructions for use do not represent all medically acceptable protocols, nor are they intended as a substitute for the physician's experience and judgment in treating any specific patient.

- Use standard hospital protocols when applicable.

- Strict aseptic technique must be used during insertion, maintenance, and catheter removal procedures. Provide a sterile operative field. The Operating Room is the preferred location for catheter placement. Use sterile drapes, instruments, and accessories. Shave the skin above and below the insertion site. Perform surgical scrub. Wear gown, cap, gloves, and mask. Have patient wear mask.

- The selection of the appropriate catheter length is at the sole discretion of the physician. To achieve proper tip placement, proper catheter length selection is important. Routine x-ray should always follow the initial insertion of this catheter to confirm proper placement prior to use.

- Administer sufficient local anesthetic to completely anesthetize the insertion site.


- Make a small incision at the exit site on the chest wall approximately 8 – 10 cm below the clavicle. Make a second incision above and parallel to the first, at the insertion site. Make the incision at the exit site wide enough to accommodate the cuff, approximately 1 cm.

- Use blunt dissection to create the subcutaneous tunnel opening. Attach the catheter to the trocar (a slight twisting motion may be helpful). Slide catheter tunneling sleeve over the catheter making certain that the sleeve covers the distal tip of the catheter. Insert the trocar into the exit site and create a short subcutaneous tunnel. Do not tunnel through muscle. The tunnel should be made with care in order to prevent damage to surrounding vessels.

Warning: Do not over-expand subcutaneous tissue during tunneling. Over-expansion may delay/prevent cuff in-growth.

- Lead catheter into the tunnel gently. Do not pull or tug the catheter tubing. If resistance is encountered, further blunt dissection may facilitate insertion. Remove the catheter from the trocar with a slight twisting motion to avoid damage to the catheter.

Caution: Do not pull tunneler out at an angle. Keep tunneler straight to prevent damage to catheter tip.



Note: A tunnel with a wide gentle arc lessens the risk of kinking. The tunnel should be short enough to keep the Y-hub of the catheter from entering the exit site, yet long enough to keep the cuff 2 cm (minimum) from the skin opening.

- Irrigate catheter with saline, then clamp catheter extensions to assure that saline is not inadvertently drained from lumens. Use clamps provided.

Caution: Do not clamp the dual lumen portion of the catheter. Clamp only the extensions. Do not use serrated forceps, use only the in-line clamps provided.

- Insert the introducer needle with attached syringe into the target vein. Aspirate to insure proper placement.


- Remove the syringe and place thumb over the end of the needle to prevent blood loss or air embolism. Draw flexible end of guidewire back into advancer so that only the end of the guidewire is visible. Insert advancer's distal end into the needle hub. Advance guidewire with forward motion into and past the needle hub into the target vein.

Caution: The length of the wire inserted is determined by the size of the patient. Monitor patient for arrhythmia throughout this procedure. The patient should be placed on a cardiac monitor during this procedure. Cardiac arrhythmias may result if guidewire is allowed to pass into the right atrium. The guidewire should be held securely during this procedure.


- Remove needle, leaving guidewire in the target vein. Enlarge cutaneous puncture site with scalpel.

Captive® J-Straightener Use Instructions


- Grasp the shoulder of the Captive® J-Straightener between the forefinger and thumb.



- Gently pull on the Captive® J-Straightener shoulder until it is just removed from the dispenser tubing.



- Holding the guidewire and the shank of the Captive® J-Straightener, fully withdraw the guidewire from the dispenser.



Caution: DO NOT grasp and pull the guidewire prior to releasing the Captive® J-Straightener. Damage to the guidewire may occur if it is pulled against the restraint of the Captive® J-Straightener.

Cautions:

- The Valved Peelable Introducer Sheath is designed to reduce blood loss and the risk of air intake but it is not a hemostasis valve.

- It is not intended to create a complete two-way seal nor is it intended for arterial use.

- The valve will substantially reduce air intake. At -12 mm Hg vacuum pressure the Valved Peelable Introducer Sheath may allow up to 4cc/sec of air to pass through the valve.

- The valve will substantially reduce the rate of blood flow but some blood loss through the valve may occur.

- Remove the dilator from the sheath and slide the valve over the sheath opening. Insert the dilator through the valve and lock in place using the rotating collar.



- Advance the introducer/dilator assembly over the guidewire and into the vein.

Note: If alternate sheath is used, follow manufacturer's instructions.


Caution: Never leave sheath in place as an indwelling catheter. Damage to vein will occur.

- Remove the dilator and guidewire from the introducer/dilator assembly by unlocking the rotating collar and gently withdrawing the dilator from the sheath.

Note: If the procedure does not allow the use of a valve, slide the valve away from the sheath opening and use as a standard sheath.



- Advance distal tip of catheter through the valve. To prevent kinking the catheter, it may be necessary to advance in small steps by grasping the catheter close to the sheath.




- After the catheter has been positioned, crack the sheath handle in half.

- Peel the non-valved side of the handle partially away from the catheter.

- Near the valve, hold the catheter firmly in position and pull the valve off of the catheter.

Note: It is normal to experience some resistance while pulling the catheter through the slit on the valve.



Caution: Do not pull apart the portion of the sheath that remains in the vessel. To avoid vessel damage, pull back the sheath as far as possible and tear the sheath only a few centimeters at a time.

- Remove the sheath from the patient.

- Confirm proper tip placement and make any adjustments to catheter under fluoroscopy. The distal tip should be positioned at the level of the caval atrial junction or into the right midatrium to ensure optimal blood flow.

Note: Femoral Catheter tip placement is recommended at the junction of the iliac vein and the inferior vena cava.

Caution: Failure to verify catheter placement may result in serious trauma or fatal complications.

- Attach syringes to both extensions and open clamps. Blood should aspirate easily from both arterial and venous sides. If either side exhibits excessive resistance to blood aspiration, the catheter may need to be rotated or repositioned to obtain adequate blood flows.

- Once adequate aspiration has been achieved, both lumens should be irrigated with saline filled syringes using quick bolus technique. Assure that extension clamps are open during irrigation procedure.

- Close the extension clamps, remove the syringes, and place an injection cap on each luer lock connector. Avoid air embolism by keeping extension tubing clamped at all times when not in use and by aspirating then irrigating the catheter with saline prior to each use. With each change in tubing connections, purge air from the catheter and all connecting tubing and caps.

- To maintain patency, a heparin lock must be created in both lumens. Refer to hospital heparinization guidelines.

Caution: Assure that all air has been aspirated from the catheter and extensions. Failure to do so may result in air embolism.

- Once the catheter is locked with heparin, close the clamps and install injection caps onto the extensions' female luers.

CATHETER SECUREMENT AND WOUND DRESSING:

- Suture insertion site closed. Suture the catheter to the skin using the suture wing. Do not suture the catheter tubing.

Caution: Care must be taken when using sharp objects or needles in close proximity to catheter lumen. Contact from sharp objects may cause catheter failure.

- Cover the insertion and exit site with an occlusive dressing.

- Catheter must be secured/sutured for entire duration of implantation.

- Record catheter length and catheter lot number on patient's chart.

HEMODIALYSIS TREATMENT

- The heparin solution must be removed from each lumen prior to treatment to prevent systemic heparinization of the patient. Aspiration should be based on dialysis unit protocol.

- Before dialysis begins all connections to catheter and extracorporeal circuits should be examined carefully.

- Frequent visual inspection should be conducted to detect leaks to prevent blood loss or air embolism.

- If a leak is found, the catheter should be clamped immediately.

Caution: Only clamp catheter with in-line clamps provided.

- Necessary remedial action must be taken prior to the continuation of the dialysis treatment.

Note: Excessive blood loss may lead to patient shock.

- Hemodialysis should be performed under physician's instructions.

HEPARINIZATION

- If the catheter is not to be used immediately for treatment, follow the suggested catheter patency guidelines.

- To maintain patency between treatments, a heparin lock must be created in each lumen of the catheter.

- Follow hospital protocol for heparin concentration.

- Draw heparin into two syringes, corresponding to the amount designated on the arterial and venous extensions. Assure that the syringes are free of air.

Catheter Length	Priming Volumes	
	Lumen	
	Arterial (ml)	Venous (ml)
20 cm	1.8	2.0
22 cm	1.9	2.0
24 cm	2.0	2.1
28 cm	2.2	2.3
32 cm	2.4	2.4
36 cm	2.5	2.6
40 cm	2.7	2.8
48 cm	3.1	3.2
55 cm	3.4	3.5

- Remove injection caps from the extensions.

- Attach a syringe containing heparin solution to the female luer of each extension.

- Open extension clamps.

- Aspirate to insure that no air will be forced into the patient.

- Inject heparin into each lumen using quick bolus technique.

Note: Each lumen should be completely filled with heparin to ensure effectiveness.

- Close extension clamps.

Caution: Extension clamps should only be open for aspiration, flushing, and dialysis treatment.

- Remove syringes.

- Attach a sterile injection cap onto the female luers of the extensions.

- In most instances, no further heparin is necessary for 48-72 hours, provided the lumens have not been aspirated or flushed.

SITE CARE

- Clean skin around catheter. Cover the exit site with occlusive dressing and leave extensions, clamps, and caps exposed for access by staff.

- Wound dressings must be kept clean and dry.

Caution: Patients must not swim, shower, or soak dressing while bathing.

- If profuse perspiration or accidental wetting compromises adhesion of dressing, the medical or nursing staff must change the dressing under sterile conditions.

CATHETER PERFORMANCE

Caution: Always review hospital or unit protocol, potential complications and their treatment, warnings, and precautions prior to undertaking any type of mechanical or chemical intervention in response to catheter performance problems.

Warning: Only a physician familiar with the appropriate techniques should attempt the following procedures.

INSUFFICIENT FLOWS:

The following may cause insufficient blood flows:

- Occluded arterial hole due to clotting or fibrin sheath.

Solutions include:

- Chemical intervention utilizing a thrombolytic agent.

MANAGEMENT OF ONE-WAY OBSTRUCTION:

One-way obstructions exist when a lumen can be flushed easily but blood cannot be aspirated. This is usually caused by tip malposition.

One of the following adjustments may resolve the obstruction:

- Reposition catheter.

- Reposition patient.

- Have patient cough.

- Provided there is no resistance, flush the catheter vigorously with sterile normal saline to try to move the tip away from the vessel wall.

INFECTION:

Caution: Due to the risk of exposure to HIV (Human Immunodeficiency Virus) or other blood borne pathogens, health care professionals should always use Universal Blood and Body Fluid Precautions in the care of all patients.

- Sterile technique should always be strictly adhered to.


- Clinically recognized infection at a catheter exit site should be treated promptly with the appropriate antibiotic therapy.

- If a fever occurs in a patient with a catheter in place, take a minimum of two blood cultures from a site distant from catheter exit site. If blood culture is positive, the catheter must be removed immediately and the appropriate antibiotic therapy initiated. Wait 48 hours before catheter replacement. Insertion should be made on opposite side of original catheter exit site, if possible.

GUIDEWIRE WEAVE TECHNIQUE

Caution: Guidewire weave should only be performed by a physician familiar with this technique.

- Advance guidewire with forward motion through the introducer needle into the target vein.
- Remove needle leaving the guidewire in the target vein.
- Thread dilator(s) over guidewire into the vein (a slight twisting motion may be used). Remove dilator(s) when vein is sufficiently dilated leaving the guidewire in place.
- Thread the proximal end of the guidewire into the distal tip of the venous lumen and back out of the slot located on the venous lumen as shown in the figure.



- Once the guidewire exits the slot in the venous lumen, thread the guidewire into the slot located on the arterial lumen as shown in the figure and advance the catheter until the guidewire exits through the red luer connector at the proximal end of the catheter.

- Once the catheter is threaded onto the guidewire, hold the proximal end of the guidewire securely and advance the catheter over it into the vein until proper placement is achieved.

Caution: Do not advance guidewire with catheter into the vein. Cardiac arrhythmias may result if guidewire is allowed to pass into the right atrium. The guidewire should be held securely during this procedure.

- Gently remove the guidewire leaving catheter in place.

- Make any adjustments to catheter under fluoroscopy. The venous distal tip should be positioned at the level of the caval atrial junction or into the right atrium to ensure optimal blood flow.

- Continue with step #23 under Seldinger Insertion Section.

CATHETER REMOVAL

Warning: Only a physician familiar with the appropriate techniques should attempt the following procedures.

Caution: Always review hospital or unit protocol, potential complications and their treatment, warnings, and precautions prior to catheter removal.

- Palpate the catheter exit tunnel to locate the cuff.

- Administer sufficient local anesthetic to exit site and cuff location to completely anesthetize the area.

- Cut sutures from suture wing. Follow hospital protocol for removal of skin sutures.

- Make a 2 cm incision over the cuff, parallel to the catheter.

- Dissect down to the cuff using blunt and sharp dissection as indicated.

- When visible, grasp cuff with clamp.

- Clamp catheter between the cuff and the insertion site.

- Cut catheter between cuff and exit site. Withdraw internal portion of catheter through the incision in the tunnel.

- Remove remaining section of catheter (i.e. portion in tunnel) through the exit site.

Caution: Do not pull distal end of catheter through incision as contamination of wound may occur.

- Apply pressure to proximal tunnel for approximately 10-15 minutes or until bleeding stops.


- Suture incision and apply dressing in a manner to promote optimal healing.

- Check catheter integrity for tears and measure catheter when removed. It must be equal to the length of catheter when it was inserted.

Flow vs. Pressure Data

Catheter Length (cm)	Pressure at flow (mm Hg)					
	400ml/min		300 ml/min		200 ml/min	
	A	V	A	V	A	V
20 cm Straight	133.5	128.5	90.2	94.2	60.0	53.2
22 cm Straight	135.1	130.1	93.7	94.8	62.8	54.5
24 cm Straight	137.1	135.5	97.5	96.6	65.3	56.2
28 cm Straight	142.6	150.9	101.1	106.2	69.4	62.6
32 cm Straight	159.9	154.4	109.7	110.0	74.6	64.5
36 cm Straight	155.4	163.6	119.0	115.7	78.6	68.6
40 cm Straight	172.9	175.5	123.1	124.8	82.6	75.0
48 cm Straight	196.4	199.6	137.9	137.7	94.4	85.5
55 cm Straight	196.9	213.3	142.7	150.1	99.9	93.1

NOTE: FLOW TESTING REPRESENTS LABORATORY RESULTS FROM SIMULATED USE TESTING

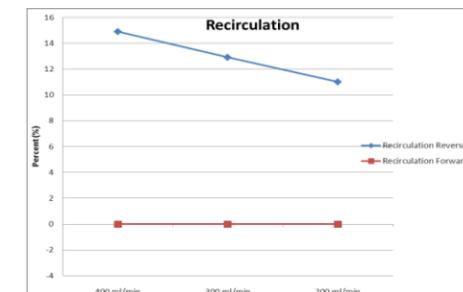

NOTE: RECIRCULATION REPRESENTS LABORATORY RESULTS FROM SIMULATED USE TESTING

Valved Peelable Introducer Sheath covered under the following U.S. Patent: #6,712,789. Foreign counterparts pending.

ANGIODYNAMICS, and Durathane are registered trademarks of ANGIODYNAMICS, Inc.

DuraFlow is a trademark of ANGIODYNAMICS, Inc.

Captive is a registered trademark of Lake Region Manufacturing, Inc.

©STORE IN A COOL DRY PLACE©PROTECT FROM UV LIGHT©



Kit contents will include (1) Hemodialysis Catheter and accessories. For exact kit contents refer to the product label.

ANGIODYNAMICS®

603 Queensbury Ave.
Queensbury, NY 12804 USA
Phone: 518-798-1215
Fax: 518-798-1360

IC 431 Rev. B